

Fig. 1

ID: white powder
Step : 0.050° Cnt Time: 1.000 Sec.
Range: 2.00 - 40.00 (Deg) Cnt. Scan Rate : 3.00 Deg/min.

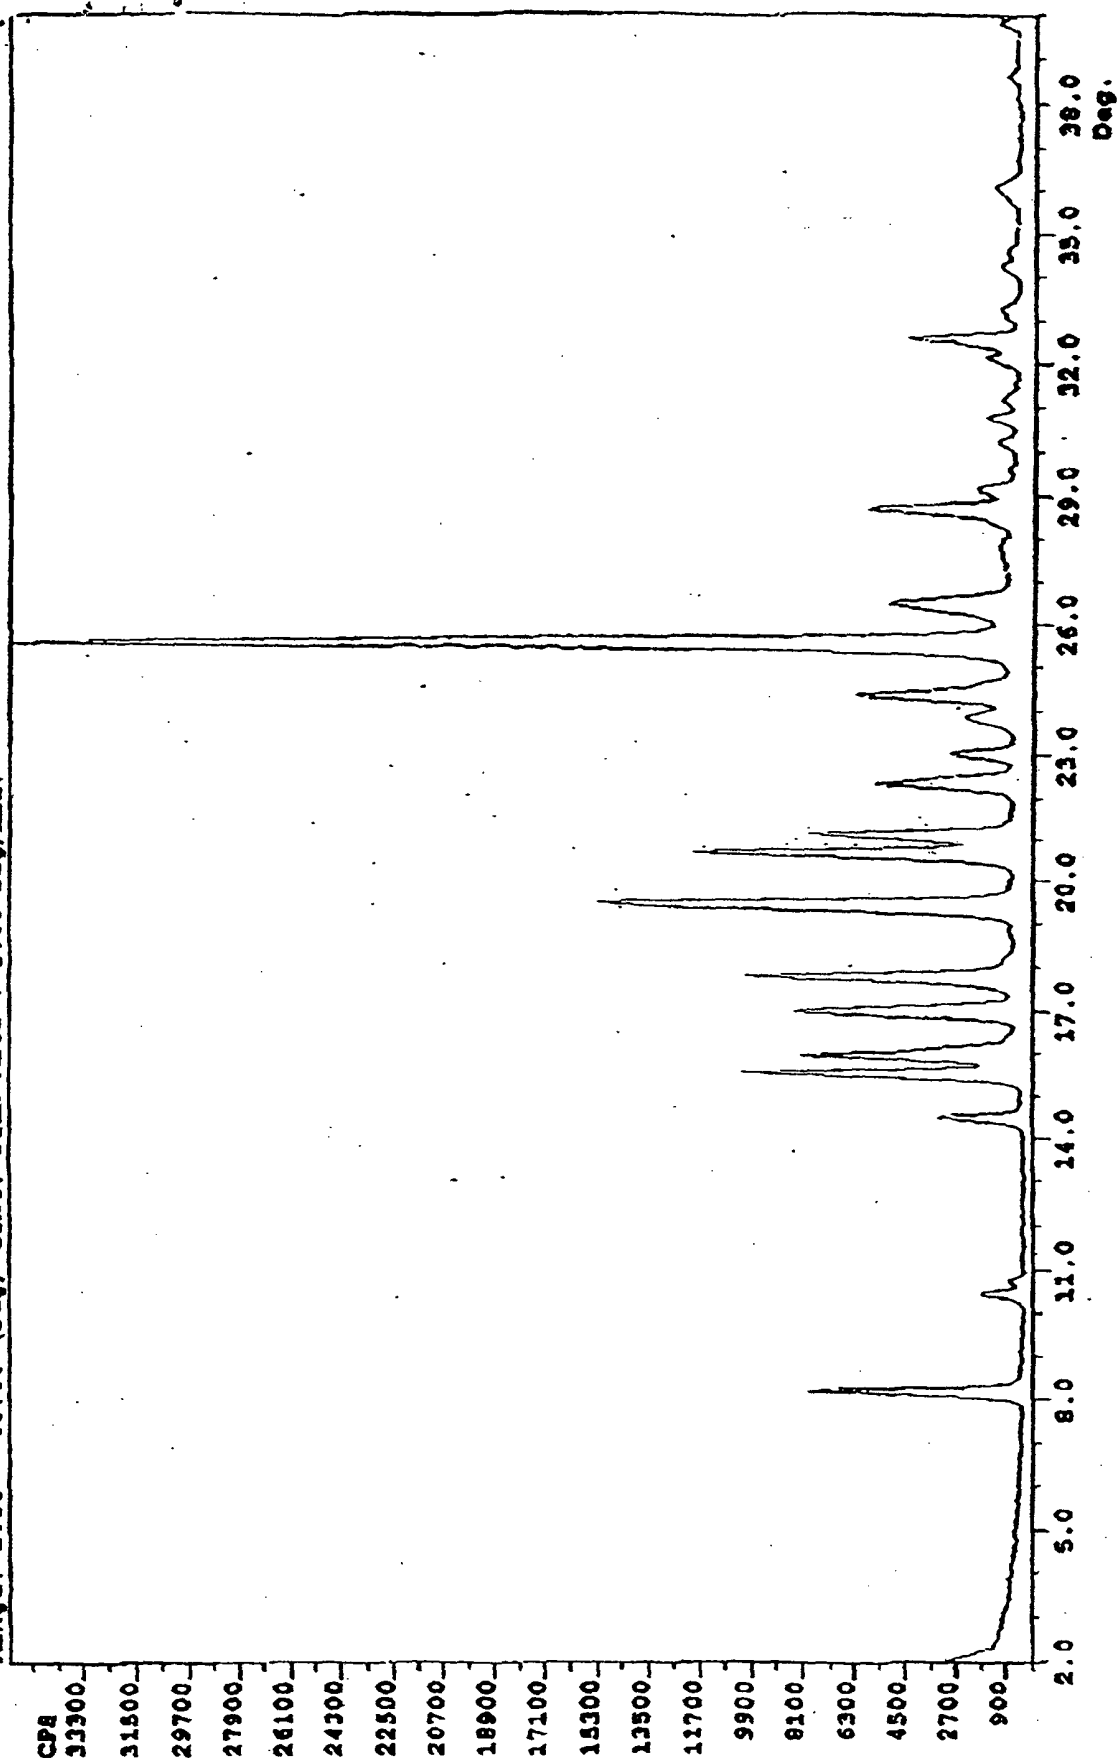


Fig. 2

Step : 0.050° Cnt Time: 1.000 Sec.
Range: 2.00 - 40.00 (Deg) Cnt. Scan Rate : 3.00 Deg/min.

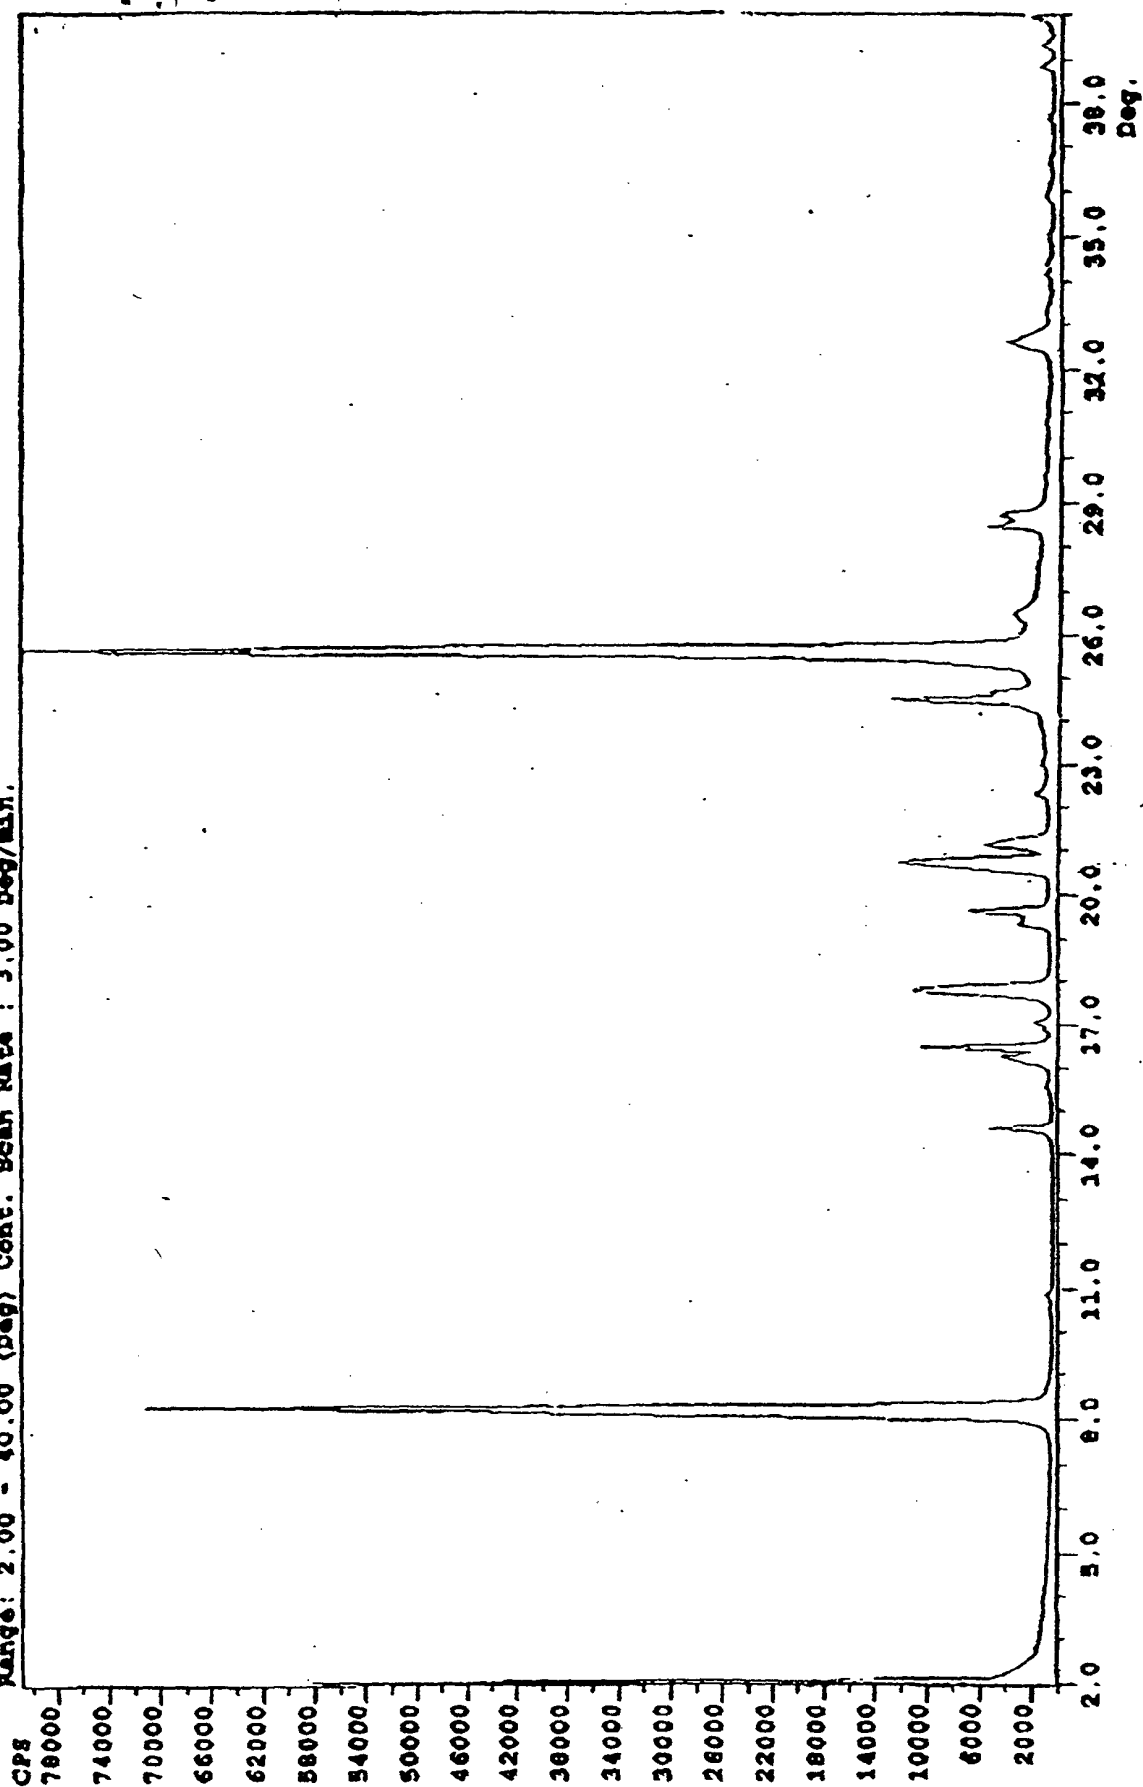


Fig. 3


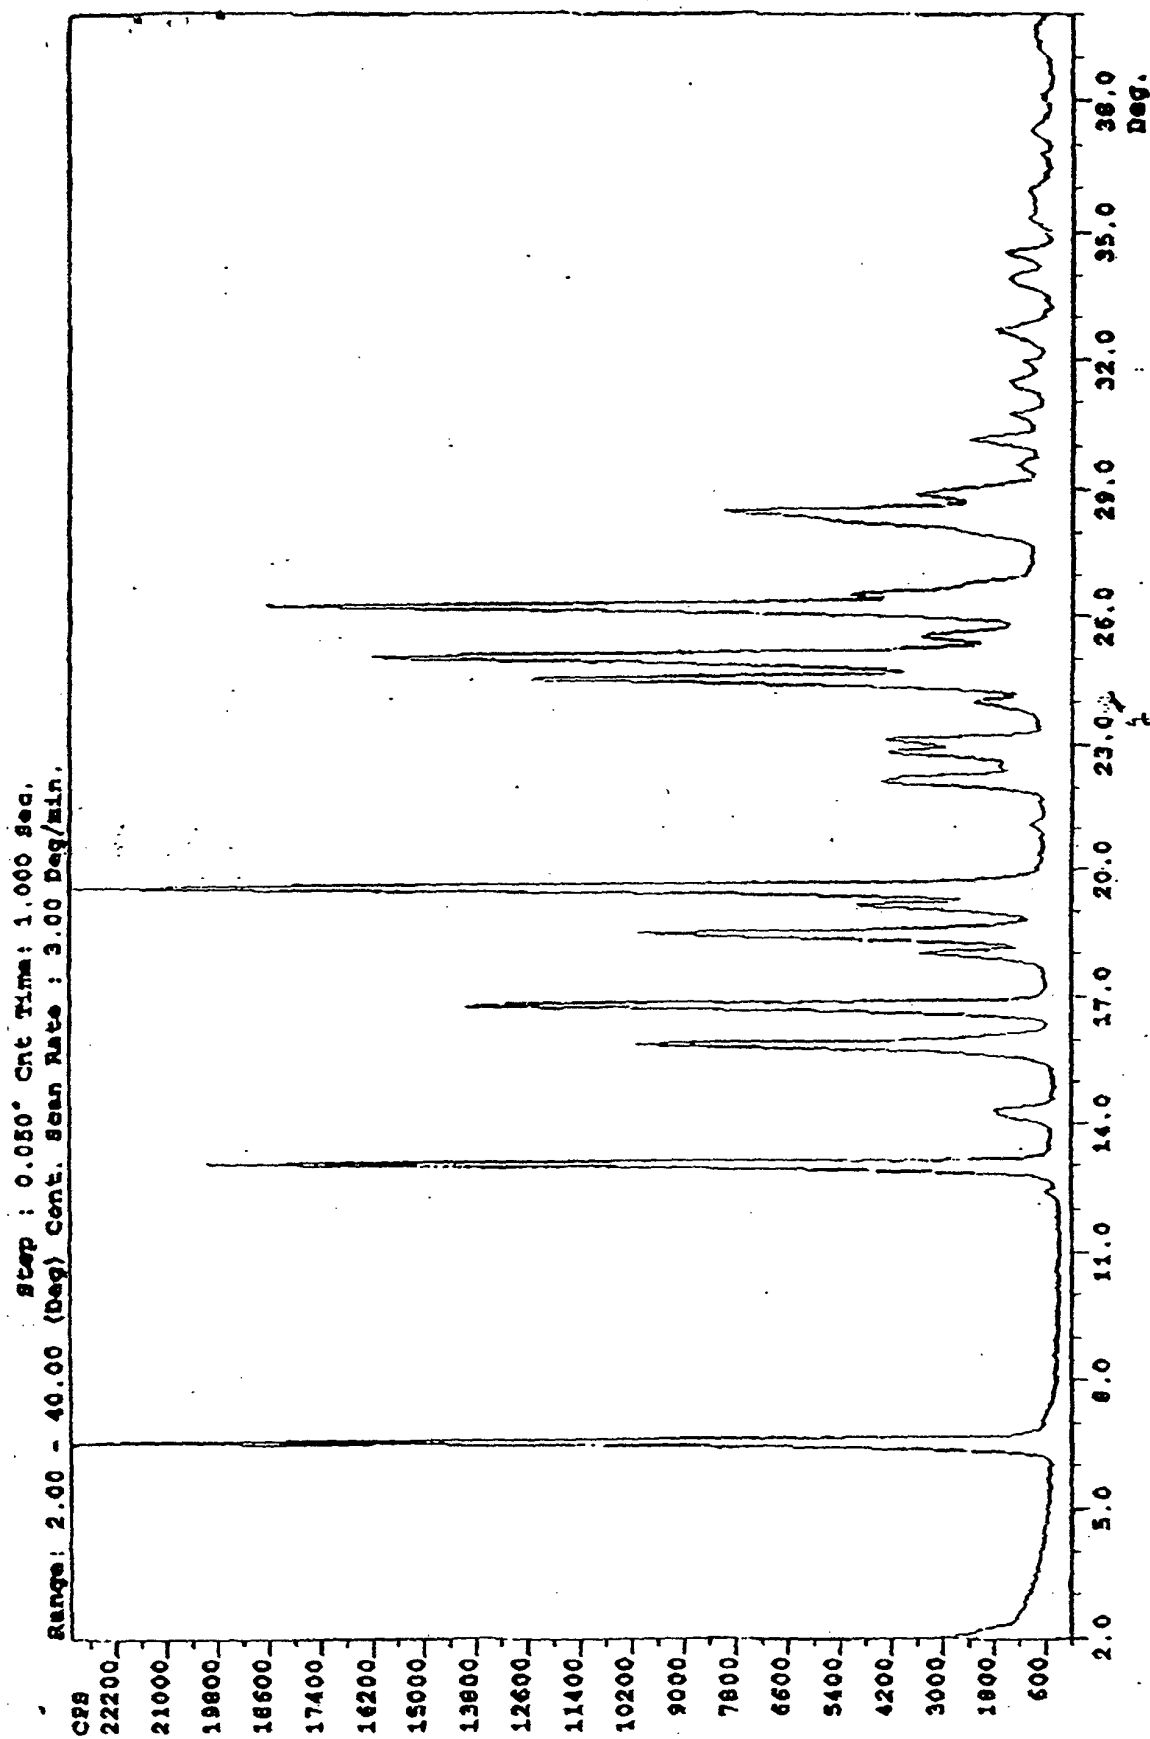


Fig. 4

Exo

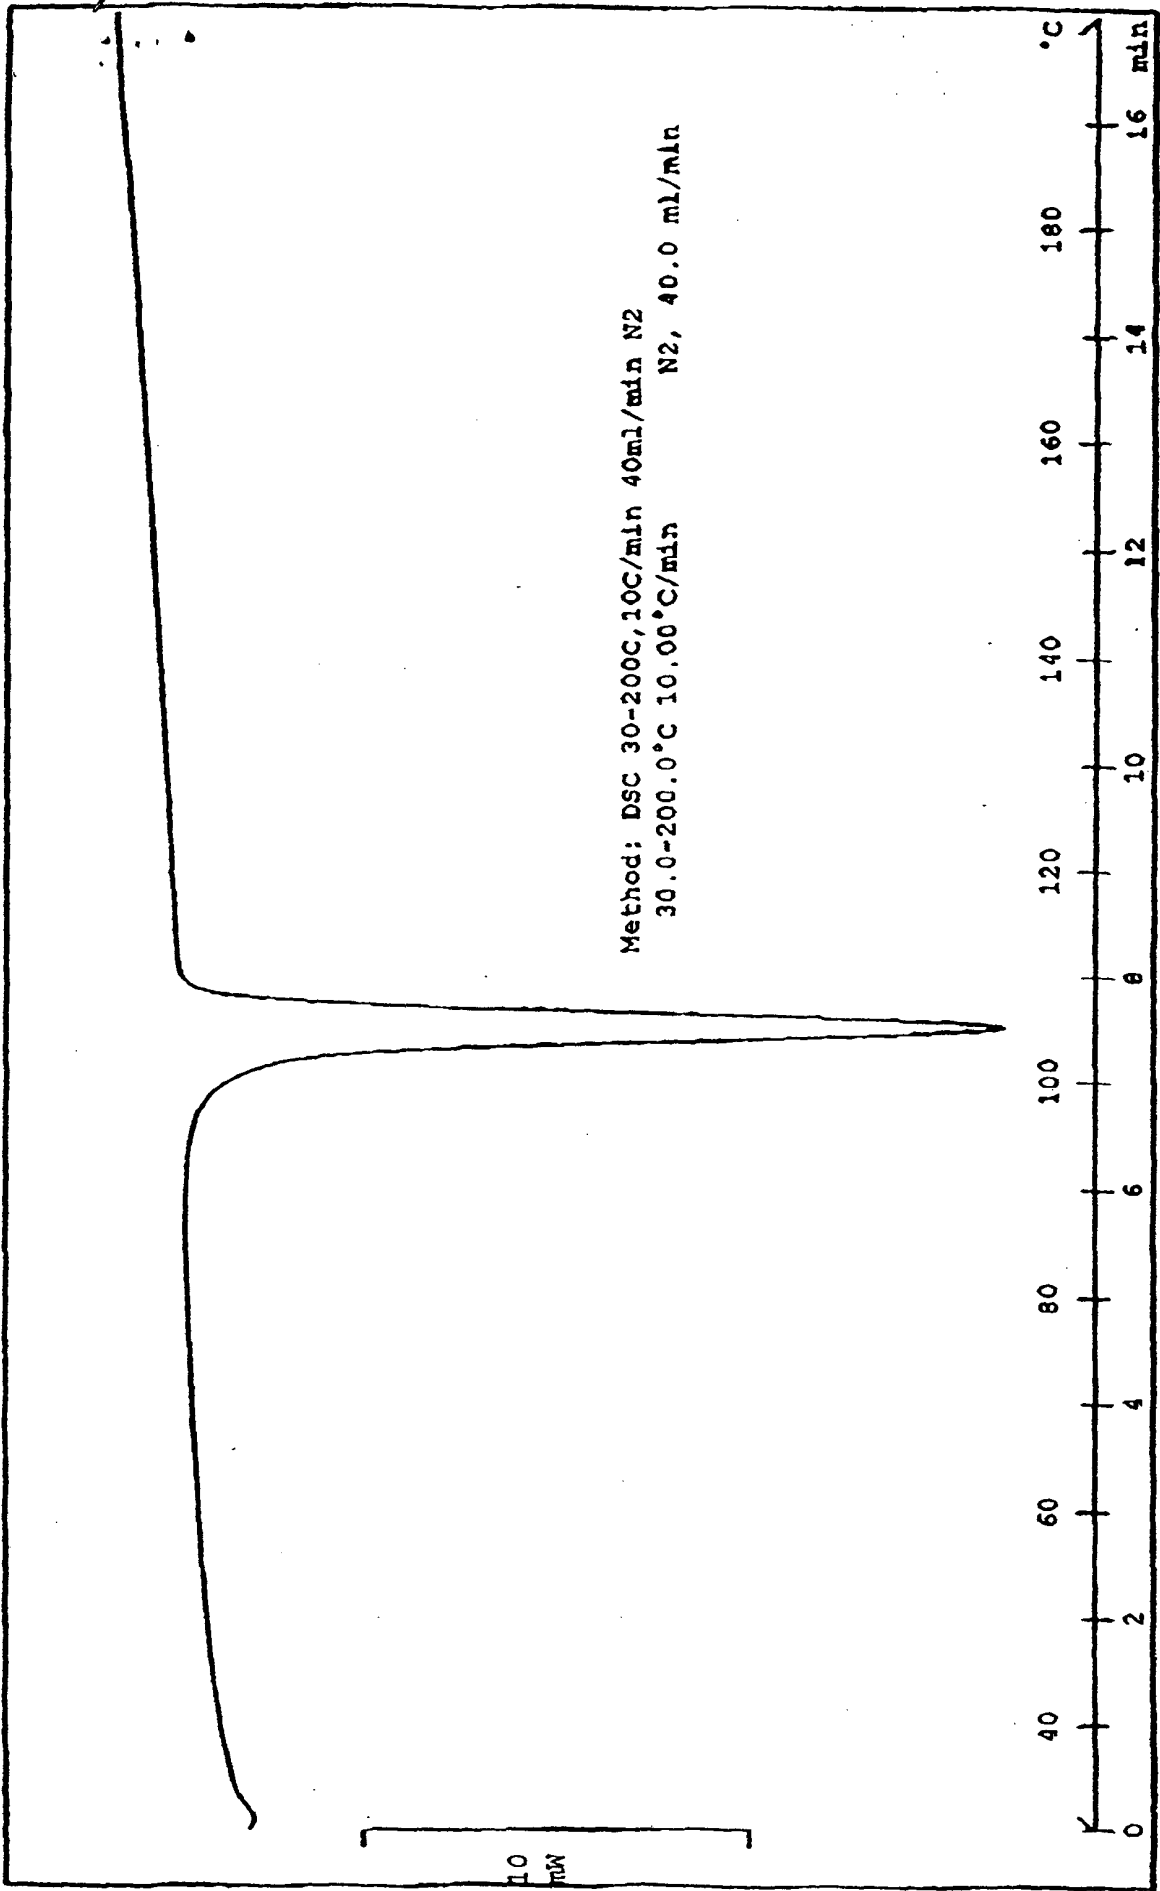

METTLER TOLEDO STAR® System

Fig 5

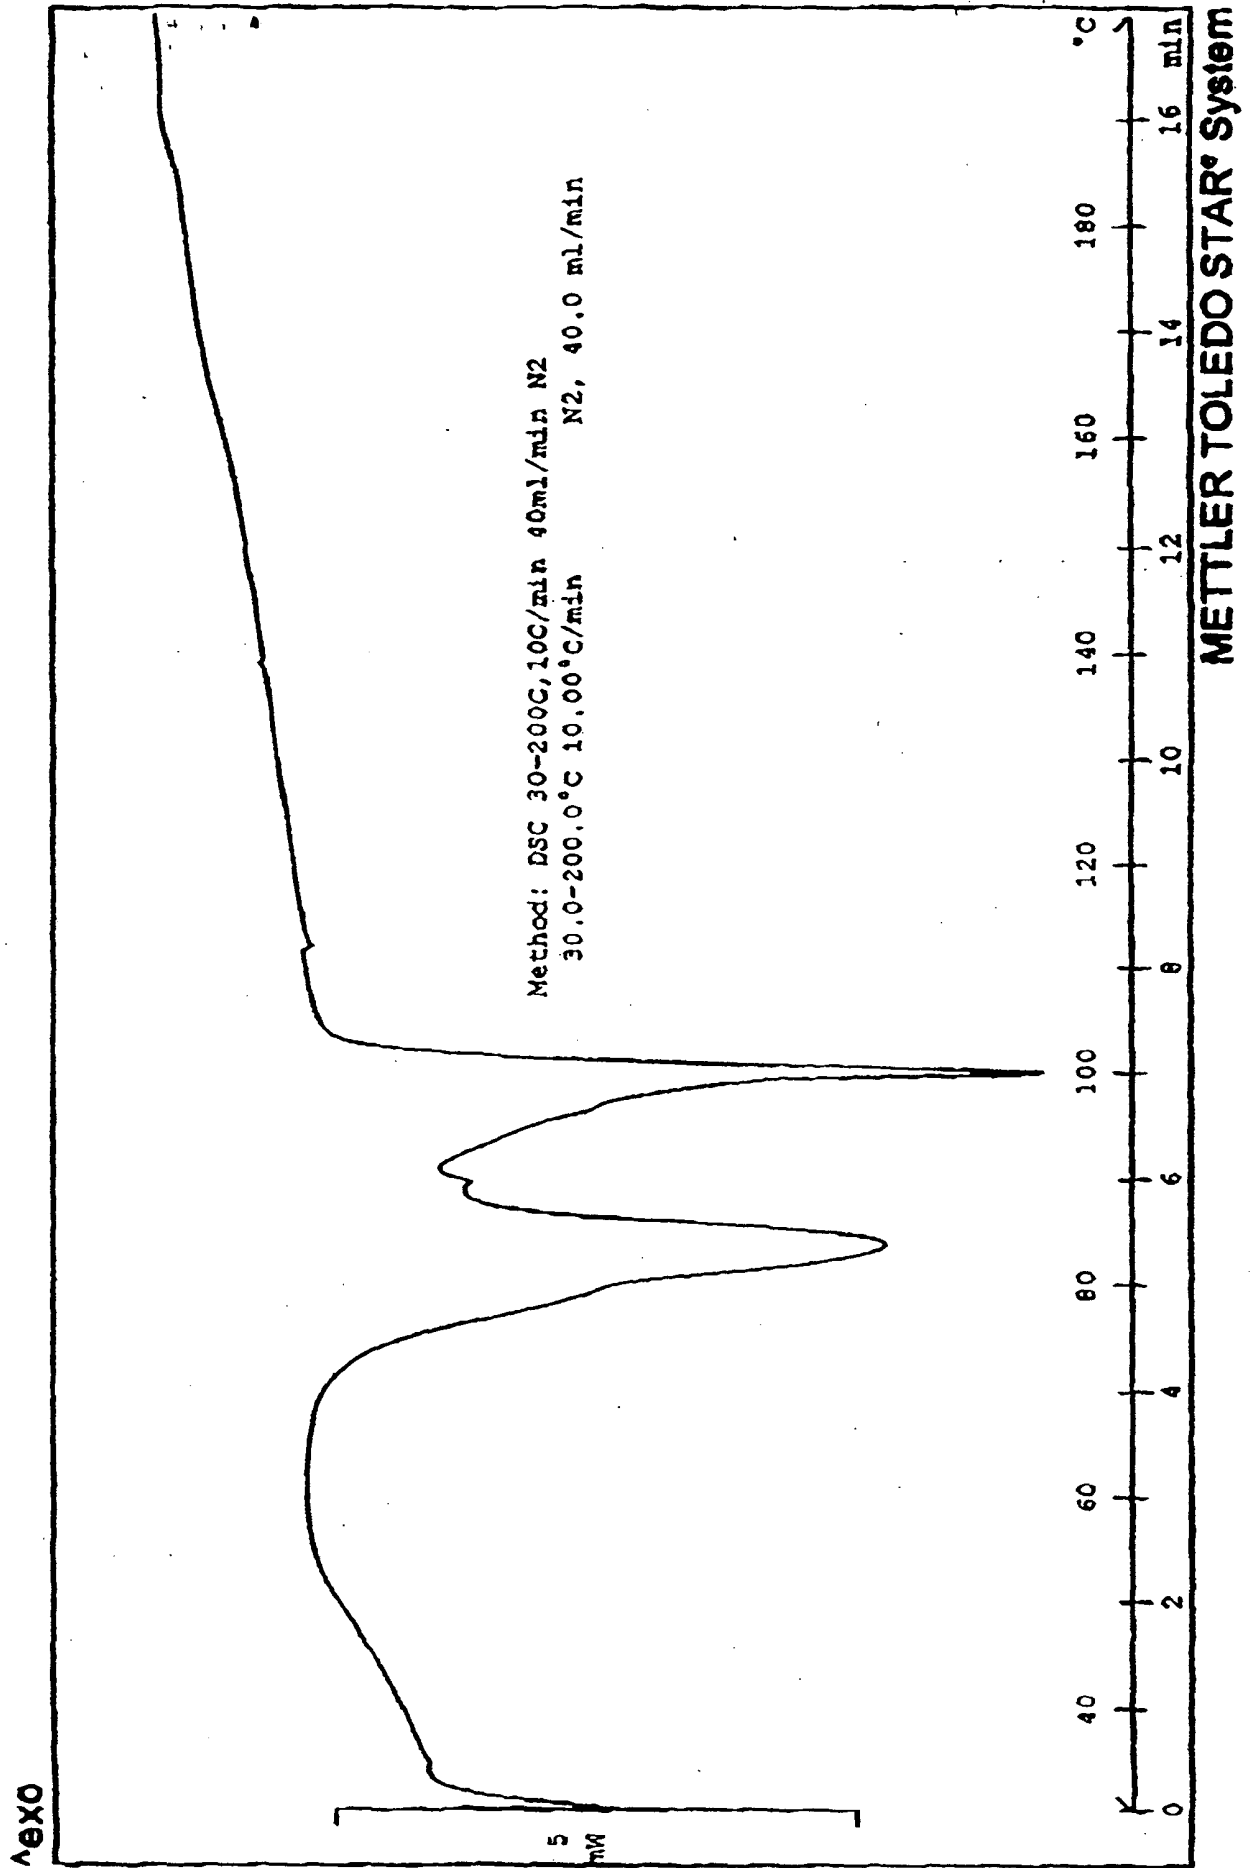


Fig. 6

